



ANALIZA BIAŁEK



100016591

Laboratory of Analysis

Client: BIO PEPTIDES
Order number: 100016591
Name: BIO PEPTIDE UK GLOW
Number of samples: 1 vial

Batch number: GLOW260
Receive date: 2026-07-24
Start date: 2026-07-30
End date: 2026-08-04

Sample identification

Substance	Method of taking a sample	Form
-----	Sample provided by customer	Blue powder in a glass vial


Results

Substance	Sample name	Content	Purity
BPC-157	BIO PEPTIDE UK GLOW 50/10/10MG	10,96mg	99%
TB-500	BIO PEPTIDE UK GLOW 50/10/10MG	9,82mg	99%
GHK-Cu	BIO PEPTIDE UK GLOW 50/10/10MG	53,01mg	99%

Research comment

The test sample was applied in the amount of 3 μ l to the BioBasic 8 Thermo Scientific column. During the course of the analysis with the method a linear gradient in the solutions of H₂O and Acetonitrile with the addition of 0.1% trifluoroacetic acid, a peaks of the sought substances appeared. Its content, when compared to the reference chromatogram, show the table above. Height the measurement error is + - 0,05mg. The actual state of the sample sent before the test is presented on the photo below

Photo of the test sample

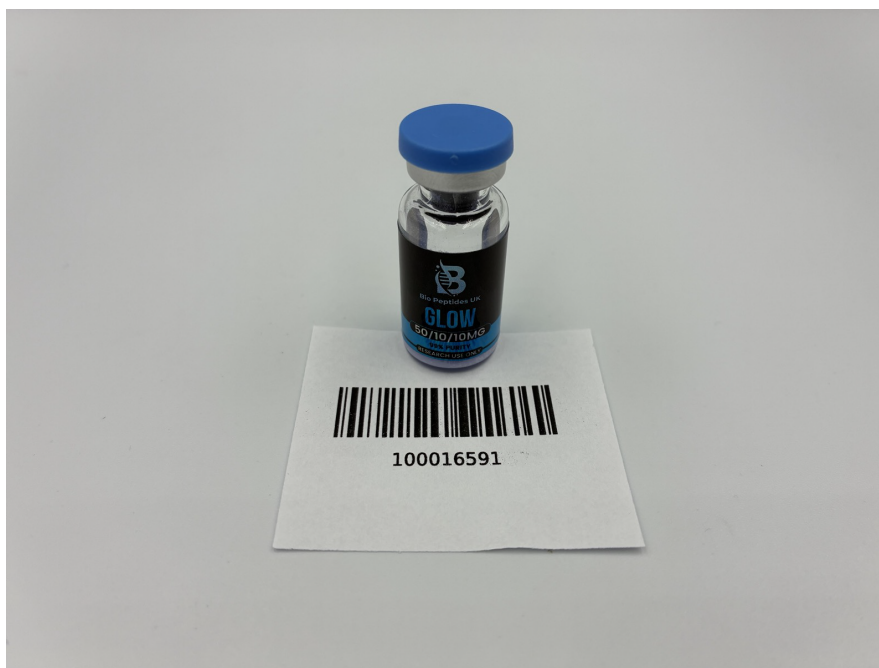

Password

5T91A8LP

Analiza Białek sp. z o.o.
KRS: 0000966168
NIP: 8992922970
REGON: 521751875

Headquarters and Laboratory:
ul. Duńska 9, 54-427 Wrocław
Budynek DELTA

Lab technician:
Analysis and research specialist
mgr Arkadiusz Zajac




ANALIZA BIAŁEK




100016591

Chromatogram

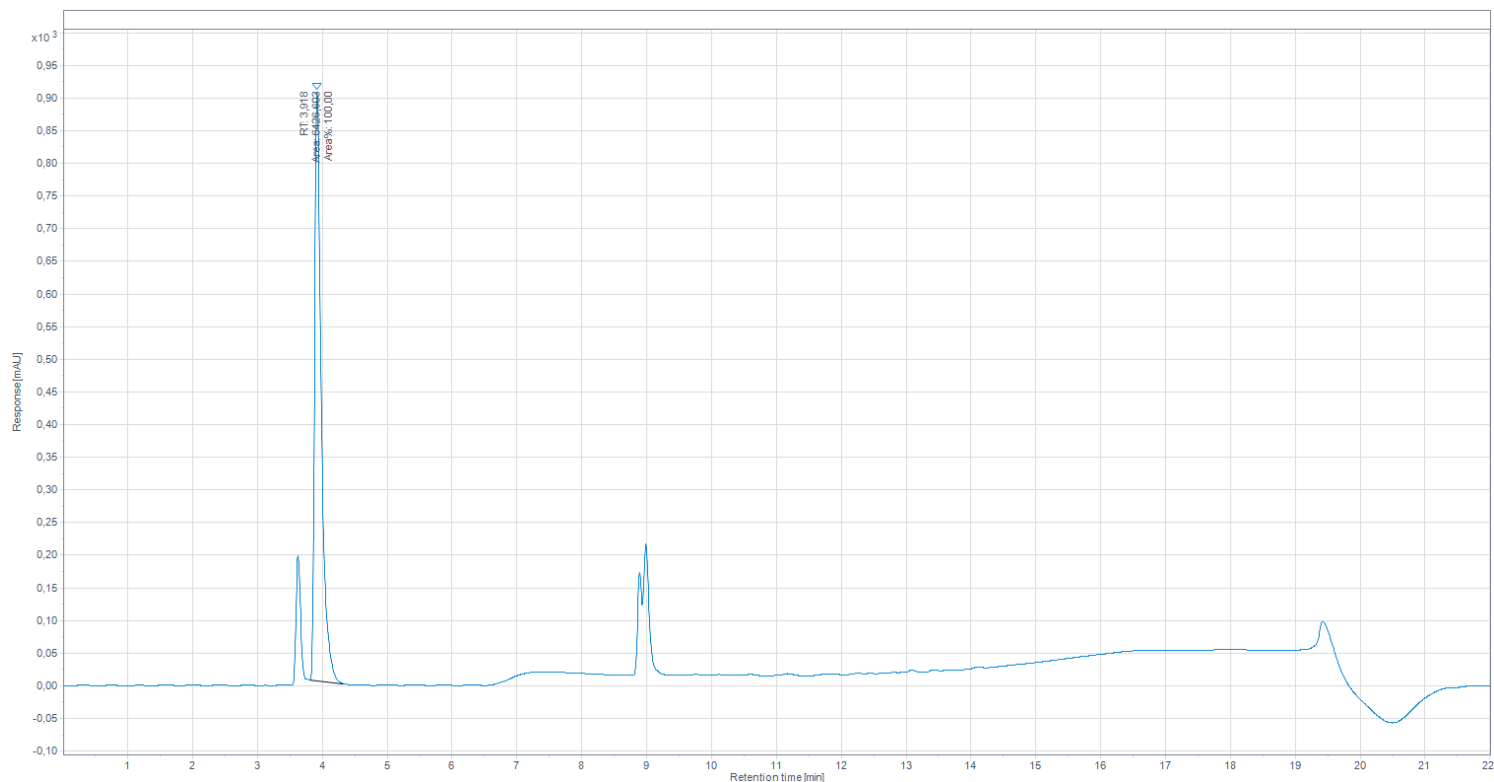

Chromatogram

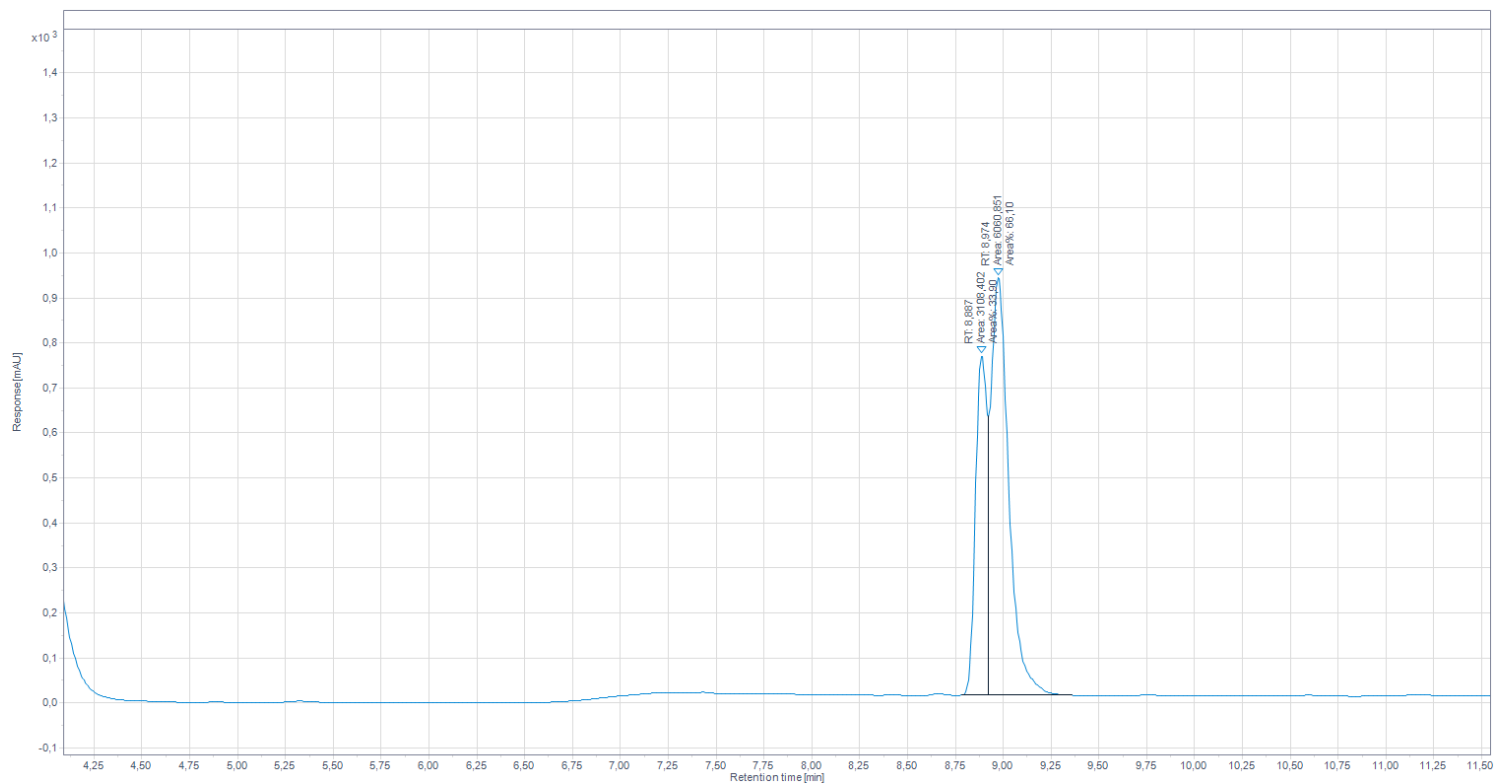

Password

5T91A8LP

Analiza Białek sp. z o.o.

KRS: 0000966168

NIP: 8992922970

REGON: 521751875

Headquarters and Laboratory:


ul. Duńska 9, 54-427 Wrocław

Budynek DELTA

Lab technician:

Analysis and research specialist

mgr Arkadiusz Zajac



ANALIZA BIAŁEK



100016591

Method

Czas	H ₂ O + 0,1% TFA	ACN + 0,1% TFA
0min	95%	5%
2min	95%	5%
12min	5%	95%
15min	5%	95%

Password

5T91A8LP

Analiza Białek sp. z o.o.

KRS: 0000966168

NIP: 8992922970

REGON: 521751875

Headquarters and Laboratory:

ul. Duńska 9, 54-427 Wrocław
Budynek DELTA

Lab technician:

Analysis and research specialist
mgr Arkadiusz Zajac