



ANALIZA BIAŁEK



100016594

Laboratory of Analysis

Client: BIO PEPTIDES
Order number: 100016594
Name: BIO PEPTIDE UK KLOW
Number of samples: 1 vial

Batch number: KLOW808
Received date: 2026-07-24
Start date: 2026-07-30
End date: 2026-08-04

Sample identification

Substance	Method of taking a sample	Form
-----	Sample provided by customer	Blue powder in glass vial


Results

Substance	Sample name	Content	Purity
BPC-157	BIO PEPTIDE UK KLOW 80MG	10,80mg	99%
TB-500	BIO PEPTIDE UK KLOW 80MG	10,00mg	99%
GHK-Cu	BIO PEPTIDE UK KLOW 80MG	54,49mg	99%
KPV	BIO PEPTIDE UK KLOW 80MG	10,78mg	99%

Research comment

The test sample was applied in the amount of 3µl to the BioBasic 8 Thermo Scientific column. During the course of the analysis with the method a linear gradient in the solutions of H2O and Acetonitrile with the addition of 0.1% trifluoroacetic acid, a peaks of the sought substances appeared. Its concentration, when compared to the reference chromatogram shows the table above. Height the measurement error is + - 0,05 mg. The actual state of the sample sent before the test is presented on the photo below

Photo of the test sample

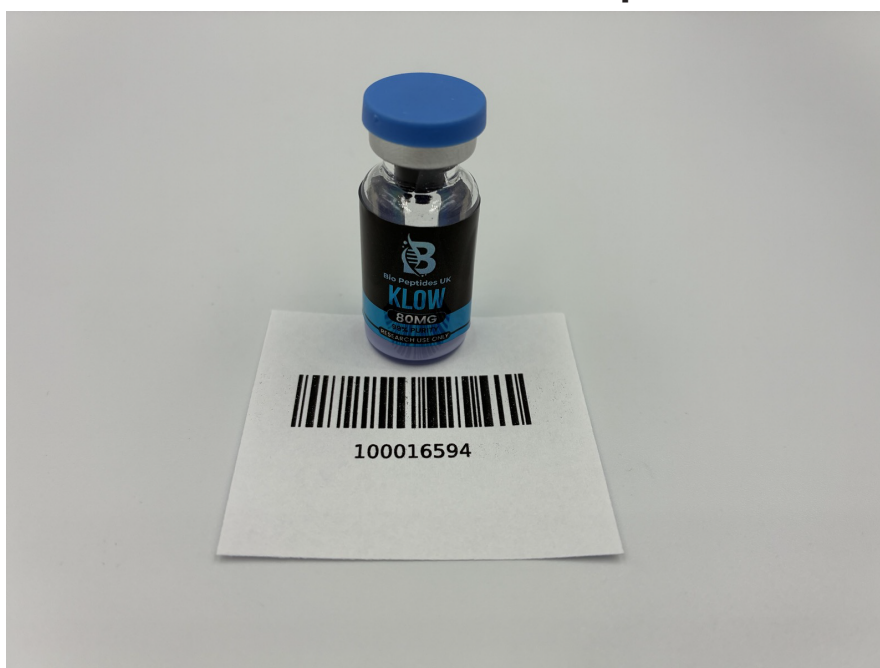

Password

A4HL13C9

Analiza Białek sp. z o.o.
KRS: 0000966168
NIP: 8992922970
REGON: 521751875

Headquarters and Laboratory:
ul. Duńska 9, 54-427 Wrocław
Budynek DELTA

Lab technician:
Analysis and research specialist
mgr Arkadiusz Zajac




ANALIZA BIAŁEK




100016594

Chromatogram

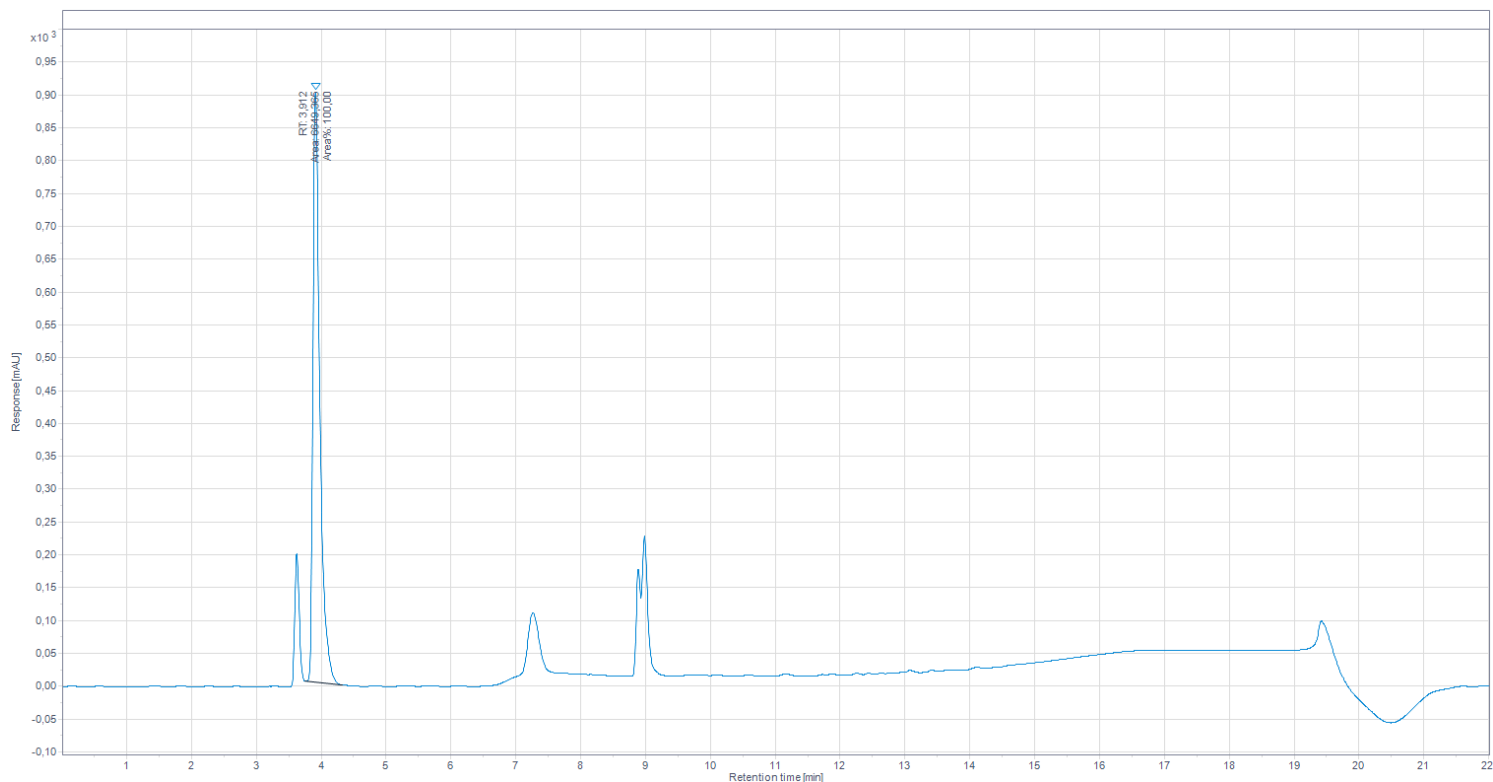

Chromatogram

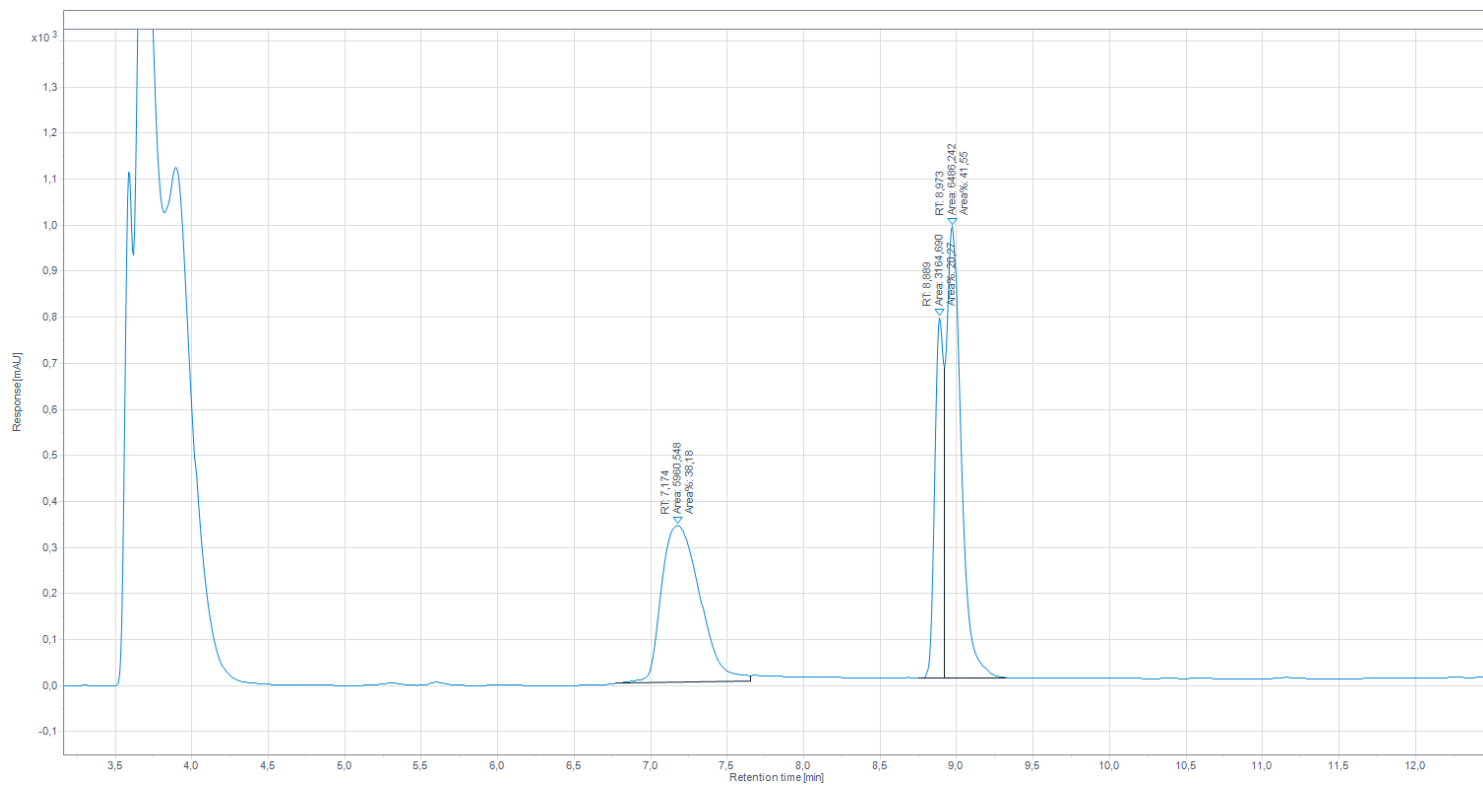

Password

A4HL13C9

Analiza Białek sp. z o.o.

KRS: 0000966168

NIP: 8992922970


REGON: 521751875

Headquarters and Laboratory:

ul. Duńska 9, 54-427 Wrocław
Budynek DELTA

Lab technician:

Analysis and research specialist
mgr Arkadiusz Zajac



ANALIZA BIAŁEK



100016594

Method

Time	H ₂ O + 0,1% TFA	ACN + 0,1% TFA
0min	60%	40%
2min	60%	40%
12min	5%	95%
15min	5%	95%

Password

A4HL13C9

Analiza Białek sp. z o.o.

KRS: 0000966168

NIP: 8992922970

REGON: 521751875

Headquarters and Laboratory:

ul. Duńska 9, 54-427 Wrocław
Budynek DELTA

Lab technician:

Analysis and research specialist
mgr Arkadiusz Zajac